




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification 4 : <b>G06K 9/00, G01B 11/14</b></p>	<p><b>A1</b></p>	<p>(11) International Publication Number: <b>WO 90/05345</b> (43) International Publication Date: 17 May 1990 (17.05.90)</p>
<p>(21) International Application Number: PCT/US89/04432 (22) International Filing Date: 10 October 1989 (10.10.89) (30) Priority data: 264,908 31 October 1988 (31.10.88) US (71) Applicant: NATHANIEL GOULD DIAGNOSTICS, INC. [US/US]; 121-B North Plains Industrial Road, Wallingford, CT 06492 (US). (72) Inventors: GOULD, Nathaniel ; 5800 Camino del Sol, Boca Raton, FL 33433 (US). FONTES, Michael ; Box 294, Route 2, Hinesburg, VT 05461 (US). THESSIN, Tyler, Reid ; 1500 Hinesburg Road, South Burlington, VT 06403 (US).</p>		<p>(74) Agents: DELIO, Anthony, P. et al.; DeLio &amp; Associates, 121 Whitney Avenue, New Haven, CT 06510 (US). (81) Designated States: AT (European patent), AU, BE (European patent), CH (European patent), DE (European patent), FR (European patent), GB (European patent), IT (European patent), JP, KR, LU (European patent), NL (European patent), SE (European patent).  <b>Published</b> <i>With international search report.</i></p>

(54) Title: PEDOTOPOGRAPHY APPARATUS AND METHOD USING MOIRE FRINGE ANALYSIS TO MEASURE FOOT SHAPES

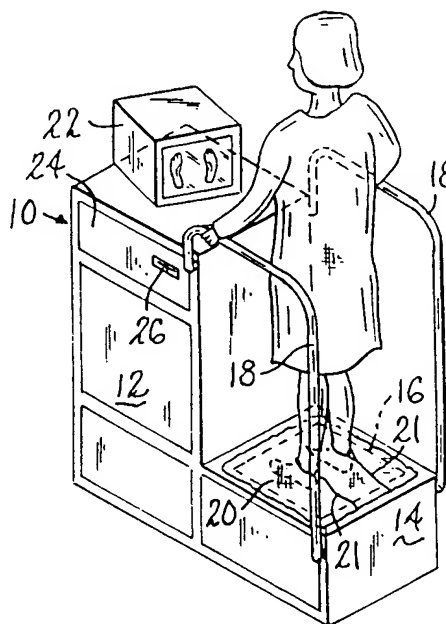

(57) Abstract

A pedotopography apparatus (10) which measures the shape of a foot by producing a moiré fringe pattern representative of the underside of the foot, capturing and storing an image of the moiré fringe pattern in an image storage buffer (24), analyzing the image to locate at least two points (A, B) of interest on the foot and computing information corresponding to the distance between the two points (A, B). In the preferred embodiment the captured image is processed by Sobel convolution to enhance edges in the image. Both an apparatus and a method of processing are disclosed.

*FOR THE PURPOSES OF INFORMATION ONLY*

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	ES	Spain	MG	Madagascar
AU	Australia	FI	Finland	ML	Mali
BB	Barbados	FR	France	MR	Mauritania
BE	Belgium	GA	Gabon	MW	Malawi
BF	Burkina Faso	GB	United Kingdom	NL	Netherlands
BG	Bulgaria	HU	Hungary	NO	Norway
BJ	Benin	IT	Italy	RO	Romania
BR	Brazil	JP	Japan	SD	Sudan
CA	Canada	KP	Democratic People's Republic of Korea	SE	Sweden
CF	Central African Republic	KR	Republic of Korea	SN	Senegal
CG	Congo	LJ	Liechtenstein	SU	Soviet Union
CH	Switzerland	LK	Sri Lanka	TD	Chad
CM	Cameroon	LJ	Luxembourg	TG	Togo
DE	Germany, Federal Republic of	MC	Monaco	US	United States of America
DK	Denmark				

-1-

DescriptionPedotopography Apparatus and Method Using  
Moiré Fringe Analysis to Measure  
5 Foot ShapesTechnical Field

This invention relates to devices for measuring the shape of a human foot. More particularly, this invention  
10 relates to devices which measure the shape of the foot by producing a moiré fringe pattern on the underside of the foot while the foot is bearing weight, and then analyze that pattern to determine the foot shape.

15 Background Art

Previous devices for measuring the shape of a foot have generally employed one of two distinct methods of operation.

The first method involves mechanically measuring the  
20 shape of the foot by making physical contact between the sides of the foot and a probe. For example, the common foot-size measurement tool found in most shoe stores generally includes a pair of blocks, one of which is fixed and one of which slides along a distance scale  
25 between them. The heel of the foot is placed in contact with the fixed block and the sliding block is pushed into contact with the toes, after which the foot length can be read from the scale. Devices employing physical contact with the foot, however, often produce  
30 measurements which vary, even when measuring the same foot, due to the compressibility of the foot tissue and the difficulty of determining the exact moment of contact.

35

-2-

The second method involves placing the foot to be measured over an array of detectors sensitive to the presence or absence of light. The foot is then illuminated from above and an outline of the foot is determined by scanning the detectors. An example of this type of device is found in U.S. Patent No. 4,538,353 issued to Gardner and the related U.S. Patent No. 4,604,807 issued to Gardner et al.

This method is an improvement over the first one in that it produces a complete foot outline, not just a single linear measurement of width or length. It also requires no physical contact with the sides of the foot which improves the repeatability of the measurements. However, it suffers from several inaccuracies of its own. The human foot does not have sides which are exactly square and perpendicular to its sole. Instead, they are curved and flare out from the portion of the sole in contact with the supporting surface. In the arch region, the sole of the foot may not be in contact with the supporting surface for a substantial distance inwards from the edge of the foot.

This three-dimensional nature of the foot permits light to leak under the edges of the foot activating the detectors and resulting in a detected foot outline which is much smaller than the actual foot. The extent of this undersizing varies depending on the foot being measured. One foot may make close contact with the supporting surface around its perimeter, or may have little or no arch thereby covering more detectors than another foot. Undersizing may also occur if the foot is not measured under load with the normal body weight applied.

This second method also suffers from problems with shadows cast by the foot and leg because of the

-3-

difficulty of providing collimated illumination from directly above the foot.

Such prior art measuring devices have generally been used to measure the foot for shoe size and width. Many  
5 times, however, one wants to measure a foot in order to construct an orthotic insert for a shoe to balance the foot to a plantigrade position.

Such inserts have previously been prepared by taking an impression of the foot in a material that permanently  
10 deforms to follow the contours of the foot, thereby producing a mold. The insert is then produced either directly in that mold or on the exterior of a second mold produced by taking a positive casting from the first mold. However, small changes in the angle of insertion  
15 of the foot into the deformable media can result in an incorrect mold, and an incorrectly shaped insert. These problems are not present when the foot is measured with the pedotopography apparatus of the present invention.

Accordingly, one object of the present invention is  
20 to provide a pedotopography apparatus which is capable of measuring dimensions of the foot at an elevation above the plane of the supporting surface while the foot is under its normal standing load.

A second object of the invention is to provide a  
25 pedotopography apparatus which is capable of measuring the arch and other features of the foot within the perimeter of the foot.

Another object of the invention is to provide a pedotopography apparatus which can record images of the  
30 foot for subsequent review and analysis.

A further object of the invention is to provide a pedotopography apparatus which can produce a foot "signature" of measured dimensions of or locations on a foot and compare that signature to a database of

-4-

previously measured feet to select an appropriately shaped shoe or insert.

#### Disclosure of Invention

5       The above, and other objects which will be apparent to those skilled in the art, are achieved in the present invention which provides a pedotopography apparatus comprising a means for producing a moiré fringe pattern representative of the topography of the underside  
10 of a foot to be analyzed. An image capture means is provided for capturing and storing an image of the moiré fringe pattern in an image storage buffer. The captured image is then provided to an image analyzing means which analyzes the image of the moiré fringe  
15 pattern to locate at least two points of interest on the foot. A computing means then calculates information, such as the length or width of the foot or the appropriate shoe size or insert, which corresponds to the distance between the two points.

20       In the preferred embodiment, the captured image is first processed by an image processing means which enhances edges in the captured image. The image processing may be performed by Sobel convolution or by other edge enhancement techniques.

25       The exact location of the points of interest may be more accurately determined by using the processed image to first identify their approximate positions and then examining the unprocessed image only in the vicinity of the approximately determined locations to find the exact  
30 location of the points.

      In the most highly preferred design, the image processing means processes only a windowed portion of the captured image, the windowed portion being restricted principally to the portion of the image containing the  
35 foot thereby reducing processing time. In the analysis

-5-

of two feet, a second windowed portion containing the image of the second foot may be mirror inverted left-for-right prior to processing so that the same processing routines may be used for both left and right  
5 subimages.

#### Brief Description of the Drawings

Figure 1 is a perspective view of the pedotopography apparatus according to the present invention.

10 Figure 2 is a side view in section of the invention showing the principle physical and optical elements of the invention.

Figure 3 is a detailed view of the light shield used to prevent extraneous light from entering the invention.

15 Figures 4a-4d show various states of the image processing of one foot.

Figure 5 shows several key points and measured dimensions on the foot.

20 Figures 6a-6c are graphical representations of the results of the image processing.

Figure 7 shows a 3 x 3 Sobel kernel used in the Sobel convolution image processing.

#### Modes for Carrying Out the Invention

25 A pedotopography apparatus according to the present invention is shown in perspective in Figure 1, generally indicated by reference numeral 10.

The principal electrical and optical components are located in the main housing 12, a portion of which projects out to form a step 14. The upper surface of the  
30 step 14 is covered by a transparent support plate 16 (seen more clearly in Figure 2) through which the underside of the foot can be viewed by the optical components within the main housing. On each side of the  
35 step portion a handrail 18 is provided permitting the

-6-

patient whose feet are to be examined to stand comfortably upon the support plate.

An opaque light shield 20 (shown in detail in Figure 3) fits around the patient's feet and prevents the patient's ankles and legs from being seen from below. The lightshield is designed to exclude extraneous light from entering the housing. It comprises an opaque fabric with two holes cut therein for the patient's legs. Slits 21 permit the shield 20 to be fitted around the patient's legs as seen in Figure 1. Closures 23 may be formed from hook and loop fasteners to hold the shield in position.

A monitor 22 is positioned on the main housing for displaying the various images of the patient's feet. Beneath the monitor, within the upper portion of the main housing, a computer 24 is mounted with a conventional removable media disk drive 26 located therein.

As described in detail below, the computer must be sufficiently powerful to handle image processing tasks. The IBM AT computer or a similar machine employing the INTEL 80286 microprocessor performs well in this application, particularly when operated with clock speeds above 8 megahertz.

The removable media disk drive 26 is preferably capable of holding at least 1 megabyte of information. Data concerning the measurements on the patient's feet can then be stored on the disk, as well as images of the feet for the patient's records.

Referring now to Figure 2, the major electrical and optical components can be seen. A light source 28 is adjustably mounted on the light source platform 30 and directs a beam of partially collimated illumination downwards through a light stop 32.

The light stop 32 includes a rectangular opening 33 therein which confines the light beam 35 to a rectangular

35



-7-

shape and prevents extraneous light from passing below the camera platform 34.

The shaped light beam 35 then strikes the illumination mirror 36 and is reflected upwards towards  
5 the foot along a light path indicated by the arrow marked by reference numeral 38. The direction the light is travelling along this light path is referred to herein as the "first direction". The first direction 38 can be varied by moving the illumination mirror 36 on an  
10 adjustable mounting 40 which permits one end of the illumination mirror 36 to be raised and lowered thereby altering the angles of incidence and reflection.

The underside of the foot is uniformly illuminated by the shaped beam 38 which passes through the transparent  
15 support plate 16. The support plate 16 has a line grating 41 formed on its surface. The grating is generally indicated by the closely spaced vertical line hatching in Figure 2 on the support plate 16. It should be understood, however, that the line grating 41 actually  
20 comprises a series of closely spaced fine parallel opaque lines which are on the surface of the support plate 16. The grating lines run across that surface in a direction which is perpendicular to the cross sectional plane of Figure 2, i.e., from the right side of the patient in  
25 Figure 1 to the left side, parallel to the front and rear edges of the support plate 16.

In the preferred embodiment, these opaque grating lines are ruled directly onto the surface of the support plate 16 which is formed of tempered glass sufficiently  
30 strong to easily support the weight of the patient. The ruled lines are preferably 0.7 mm center-to-center and 0.3 to 0.4 mm wide, however these dimensions may be varied provided that the line grating is capable of producing a moiré fringe pattern representative of  
35 the topography of the underside of the foot as described below.

-8-

Suitable gratings may also be produced by using a series of fine parallel wires suspended in a frame below the support plate 16 or through the use of a transparent film upon which opaque grating lines have been  
5 photographically reproduced.

The light beam 38, as it passes through the opaque grating lines, forms a series of shadow lines which are projected onto the underside of the foot. These shadow lines are straight wherever the foot is in contact with  
10 the support plate 16 or parallel to it and are curved along the contours of the foot wherever the surface of the foot lifts up from the support plate. The position of the shadow lines and their deviation from the straight  
15 carry information on the elevation of the foot above the support plate which can be obtained through the procedure described below.

After the light strikes the sole of the foot, it is reflected back through the grating 41 to the camera mirror 42 positioned directly beneath the foot, over to a  
20 second camera mirror 44 and up into the camera 46. In the preferred embodiment, the camera 46 is positioned pointing directly down into the second camera mirror 44 which is set at a 45° angle. Camera mirror 42 is also set at a 45° angle and thus the camera sees an image of  
25 the foot from the direction indicated by arrow 48 which is referred to herein as the "second direction". It will be noted that the second direction 48 is defined as being opposite to the direction light is travelling at this point.

30 Because the second direction 48 is substantially perpendicular to the plane of the support plate 16, the image seen by camera 46 has a uniform scale over the entire image area.

Although they are not shown, the support plate 16  
35 also has several reference points, distance scales and

-9-

window frame lines marked onto its surface which permits  
1) calibration and alignment of the system, 2)  
calculation of the scale factor between distances (in  
pixels) on the camera image and distances on the surface  
5 of the support plate, and 3) accurate placement of the  
patient's feet on the plate. After assembly of the  
apparatus, the scale factor is carefully checked to  
ensure that it is substantially constant over the entire  
image area.

10 In the preferred embodiment, the light 28 is a 100  
watt light source. At this relatively low wattage, the  
generated heat is kept to a minimum and a supplemental  
exhaust fan is not required provided that the main  
housing is properly ventilated.

15 The mirrors 36, 42 and 44 should all be of high  
quality, however, first-surface precision optical quality  
mirrors are not required and good plate glass mirrors may  
be used. The three mirrors 36, 42 and 44 are preferably  
mounted on a single tray 50 which can be removed for  
20 cleaning and adjustment of the mirrors.

As can be clearly seen in Figure 2, the camera 46  
views the foot through the grating 41 on the support  
plate 16. Thus, an undistorted image of the grating with  
straight grating lines is superimposed upon the image of  
25 the foot with the curved shadow lines. Because the first  
direction 38 is different from the second direction 48,  
the curved shadow lines carrying the elevation  
information about the foot interfere with the straight  
lines of the grating to produce a fringe pattern.

30 A fringe pattern of this type is known as a moiré  
fringe pattern. The fringes are formed along lines of  
constant elevation above the surface of the grating, with  
their spacing being determined by the grating size, the  
angle difference  $\phi$  between the first direction 38  
35 and the second direction 48 and the slope of the foot

-10-

surface. Thus, the image seen by camera 46 has the appearance of a topographic map of the foot with the topographic fringe lines appearing wherever the foot is elevated above the surface of the support plate, which occurs principally at the arch and along the perimeter of the foot.

Figure 5 shows the image of a foot as it appears to the camera 46. At the edges of the foot, where the surface of the foot is nearly perpendicular to the support plate, the fringes crowd closely together forming a dark band outlining the true outer perimeter of the foot. By locating the position of points of interest along this band, the outer dimensions of the foot can be accurately determined.

The image of the foot seen by the camera actually contains two sets of lines, namely the straight grating lines and the curved shadow lines cast by the light through the grating. The moiré fringes are an optical effect caused by the visual reinforcement which occurs wherever the two sets of lines cross. Nonetheless, the effect is such that the moiré fringes appear to be much broader, stronger and more widely spaced in the image than are the two sets of lines that form the fringes. When the image is viewed by the camera, the narrowly spaced grating lines are not fully resolved by the camera and are unnoticed in the image, and only the well-defined fringes can be clearly seen.

Although the specific means for producing the moiré fringe pattern described above is preferred due to its simplicity, other means are suitable. For example a projector may be used to project an image of the grating onto the foot from the first direction, and the camera may view the foot through another grating from the second direction. Alternatively, the second set of

-11-

grating lines may be added electronically to the image seen by the camera.

Nevertheless, regardless of how the moiré fringe pattern is produced, an image of it is finally captured  
5 and stored in an image storage buffer. In the preferred embodiment, the camera 46 images the moiré fringe pattern onto an internal array of sensors producing a digitized image that is 512 x 512 pixels in size. Computer 24 contains an image capturing system connected  
10 to camera 46 which, upon activation of a remote switch, captures and stores the image seen by the camera.

The initial unprocessed image comprises a 512 x 512 array of pixels, each pixel having a gray-scale value from zero to 255. This resolution has been found to be  
15 sufficient for the moiré fringe analysis, however cameras with other resolutions have also been found to operate satisfactorily.

To summarize the operation of the pedotopography apparatus to this point, the patient steps up onto the  
20 support plate 16 facing the main housing 12 and grasps the hand rails 18. Light shield 20 is then placed around the patient's feet to prevent outside light from entering the camera system and interfering with the measurements.

The computer system is preferably designed to  
25 continuously display the camera picture on monitor 22 so that the patient may, under the operator's directions, move his or her feet into proper alignment with the reference points marked on the support plate's surface.

Once the patient's feet are in position, the operator  
30 activates a switch or presses a button on a keyboard (not shown) which signals the computer to capture the image displayed on the monitor. That captured image contains the topographically encoded height and shape information carried by the moiré fringes, which information may

35

-12-

be determined by computerized analysis of the image as described below.

In most cases, it is not the magnitude of the height of the foot above the support plate which is the principal item of interest, but rather it is the projected location on the support plate of a point which is above the surface of the support plate which is of interest. For example, when determining the length of the foot, the tip of the longest toe will generally not be in contact with the support plate. The exact height of this point above the plate is generally not of interest, only its location over the plate needs to be known to calculate the length of the foot. As previously described, the moiré fringes delineate the maximum perimeter of the foot, including the point at the tip of the longest toe, the point at the heel, etc. Accordingly, by locating points on the perimeter fringe in the captured image and measuring the distance between them, any desired dimension, e.g., foot length, heel width, maximum foot width, etc., may be easily determined.

Whenever height information is needed, it is calculated by counting the number of fringes between the point of interest and a nearby point in contact with the supporting surface. As is well known to those familiar with moiré fringe topographic analysis, each new fringe occurs at a predetermined height above the previous fringe. That height difference is set by the relation:

30

$$h = \frac{d}{\tan \phi}$$

where h is the height difference, d is the spacing of the grating lines, and  $\phi$  is the angle between the first

35

-13-

(illumination) direction and the second (viewing) direction.

Thus, by counting the number of fringes,  $N$ , between a point in contact with the supporting surface and a point  
5 of interest, the height  $H$  of the point of interest can be determined by the relation:

$$H = N\lambda = \frac{Nd}{\tan \phi}$$

10

The disclosure below describes how each point of interest and the location of each fringe is found.

In the preferred design, after the image capture system is triggered, the computer automatically processes  
15 the image to identify points on the foot, determine distances between those points and produce an output of useful information which corresponds to those distances.

Two outputs which are commonly produced are foot length and foot width which may be displayed in units of  
20 length or in standard shoe size and width.

Preferably, additional points on the foot are measured which are related to the way in which the foot is shaped and how it bears the weight applied to it. By measuring a large number of feet, each of which is also  
25 carefully diagnosed by a trained physician, an information base can be accumulated. An unknown foot can then be measured and compared to this information base to produce an output quantizing the extent to which the foot deviates from the plantigrade status thereby assisting  
30 the physician in diagnosis and treating the foot.

Furthermore, the information base may contain a cross-reference to a standardized shoe insert or orthosis which has previously been found to balance a foot of similar measured structure to the plantigrade position.

35

-14-

Thus, another output of the measuring and analyzing process may be a code identifying a previously manufactured shoe or corrective insert which balances the foot to the neutral position. For unusual structural problems of the foot which do not correspond to previously measured and diagnosed feet in the database, the outputs may be the dimensions required to make a custom-made corrective shoe insert.

For each output, the starting point is to identify the location of points of interest on the foot. For example, Figure 5 shows a patient's right foot; seen from below in the captured image. Two points of interest are points A and B corresponding to the tip of the toes and the bottom of the heel, respectively, which are used to determine the length of the foot. The perimeter fringes run through each point and the criterion of interest is the point on the fringe at the top of the image (for point A) and the point on the fringe at the bottom of the image (for point B).

Broadly speaking, the complete process involves 1) capturing the initial image 2) analyzing the image to locate the points of interest, and 3) computing output information which corresponds to the distance between the points.

Capturing and storing the image involves rapidly scanning the entire 512 x 512 pixel image array and storing an eight bit number corresponding to the light level for that pixel. Conventional image capture systems are widely available which provide this function. The complete captured image contains images of two feet as well as some border area and the reference points on the support plate. As described below, each of the pixels in the captured image is processed in the preferred embodiment. To increase processing speed, only that



-15-

portion of the image containing the actual foot images needs to be stored. A windowed subimage of the entire image is typically stored for each foot which also reduces memory requirements in the computer 24 and  
5 storage space requirements.

The size and position of the required window may be calculated by the computer to frame each subimage of a foot wherever the foot appears in the complete image. However, it has been found to be simpler to mark the  
10 window on the surface of the support plate and have the operator ensure that the patient's feet are moved into the windows before the image is captured. Each foot subimage is typically about 100 pixels wide by 300-400 pixels high out of the full 512 x 512 image.

15 A second simplification in processing is to mirror invert the image of the left foot in a left-for-right inversion so that it appears to be the image of a right foot. This permits the same high speed image processing and analyzing routines to be used for both the left and  
20 right foot subimages.

Once the initial image is captured and the subimages extracted, they are passed individually to the image analyzer. In the preferred embodiment, this is a computer such as an IBM AT or compatible computer. Such  
25 computers, with interfaces for suitable image capturing systems, are widely available and are sufficiently fast and inexpensive enough for this application.

One method of operation of the image analyzer is the direct method. In this method, the image analyzer  
30 identifies point A at the tip of the toes by scanning each row of pixels in the foot subimage starting at the top and working down until the first row containing the foot perimeter moiré fringes is found. The pixels containing the fringes have a distinctly different

-16-

intensity level than the background permitting them to be identified by comparing the intensity of each pixel to the average background intensity.

A similar method may be used to identify the row and column numbers for point B at the heel by searching rows from the bottom up. By searching in columns from the left and right, the position of points G and E may then be found setting the width of the foot. In fact, each point on the perimeter of the foot may be identified by tracing out, pixel by pixel, the perimeter fringes from the previously identified points on that perimeter.

Unfortunately, the direct method of locating the points described above, although feasible, requires a great deal of care to avoid false detection of the location of the fringes. Random noise in the image, internal reflections in the camera or optics, etc., all produce variations in intensity of points in the image which may be mistakenly detected as the moiré fringe at the perimeter.

Substantially improved results have been found by using image processing on the captured image to enhance edges in the image thereby increasing the contrast between the edges of the fringes and the background.

Although many different edge enhancement techniques are known, including Fast Fourier Transform filtering, Roberts convolutions, and others, the present invention has been found to operate most effectively using the Sobel convolution with a 3 x 3 video kernel to enhance vertical or horizontal edges, depending upon the point being located.

Figure 7 shows a 3 x 3 kernel to enhance vertical edges used in the image processing step which is also performed by computer 24. The 3 x 3 kernel contains nine elements found in three rows ( $r_1$  to  $r_3$ ) and three

-17-

columns ( $c_1$  to  $c_3$ ) of numbers in a tic-tac-toe pattern. The vertical convolution video kernel of figure 7 is used in the following way to produce a processed image with enhanced vertical edges:

- 5           1. Select a pixel having an intensity magnitude  $p(x,y)$  in the original captured image, located at row =  $y$ , column =  $x$ .
2. Position the 3 x 3 video kernel over the selected pixel such that the central element in the kernel,  $r_2c_2$  is directly over the selected image pixel  $p(x,y)$  and the eight surrounding elements are over the eight pixels surrounding the selected pixel.
- 10           3. Multiply the numeric value in each element of the 3 x 3 kernel times the magnitude of the image pixel beneath that element.
4. Add the nine numbers obtained from the previous step to obtain a new intensity level  $p'(x,y)$  and insert that total as the intensity value at location  $(x,y)$  in a new processed image, i.e., the vertical sobel processed image.
- 20           5. Repeat the process for all of the original image pixels  $(x, y)$  to produce a complete processed image.
- 25

Specifically, the value of the pixel  $p'(x,y)$  in the processed image is:

$$\begin{aligned}
 30 \quad p'(x,y) = & r_1c_1 p(x-1,y-1) + r_1c_2 p(x,y-1) + r_1c_3 p(x+1,y-1) \\
 & + r_2c_1 p(x-1,y) + r_2c_2 p(x,y) + r_2c_3 p(x+1,y) \\
 & + r_3c_1 p(x-1,y+1) + r_3c_2 p(x,y+1) + r_3c_3 p(x+1,y+1)
 \end{aligned}$$

or, substituting the actual elements of the vertical 3 x 3  
35 kernel:

-18-

$$\begin{aligned} p'(x,y) = & p(x+1, y-1) - p(x-1, y-1) \\ & + 2 p(x+1, y) - 2 p(x-1, y) \\ & + p(x+1, y+1) - p(x-1, y+1) \end{aligned}$$

Figures 6a-6c show a two-dimensional simplified graphical representation of the results of this processing. Figure 6a represents a slice through the unprocessed subimage of one foot along one row of pixels, for example from G to F in Figure 5. The vertical scale shows the pixel intensity which ranges from 0 to 255. The horizontal scale shows the pixel position along G-F. Outside the foot the background intensity is at or near zero, and inside the interior of the foot, the intensity reaches a maximum. At the outer edge of the foot between points J and K, the pixel intensities gradually increase. An actual subimage would generally have substantially more fluctuations than the graph in Figure 6a due to the fringes and other noise which have been ignored for this description of the Sobel processing.

Referring to Figure 7 again, it will be seen that the elements in column one are equal to, but have the opposite sign as, the elements in column 3, while all the elements in column 2 are zero. Thus, wherever the unprocessed image has a uniform, unvarying intensity (which occurs in the center of the foot and in the background area), the Sobel convolution value will be zero. The positive contribution from pixels on the right side of the kernel will be exactly counteracted by the negative contribution from pixels on the left side of the kernel. This can be seen in Figure 6b between points K-L and to the left of point J and the right of point M.

However, where the pixel intensity is varying, as between J-K and between L-M in Figure 6a, the left and

-19-

right side of the kernel contribute unequally to the result. Where the original image is increasing in intensity, as between points J and K in Figure 6a, the positive contribution from the right side of the kernel outweighs the negative contribution, forming the positive "hump" between points J and K in Figure 6b. Where the value is decreasing, as between points L and M, the negative contribution outweighs the positive, forming the negative dip between L-M in Figure 6b.

10 Figure 6c shows the absolute value of the convolution results of Figure 6b which avoids the difficulty of displaying images with negative intensity values.

It can be seen in Figure 6c that the absolute convolution enhances the position of the left and right edges in the image of Figure 6a, clearly marking their positions. It is more difficult to see the manner in which random noise and fluctuations in the image are smoothed out, yet this happens also as a result of the 3 x 3 size of the video kernel, making it much easier to locate the edge positions at H and I.

While the foregoing has been described with respect to vertical Sobel convolutions, i.e., enhancement of vertical edges in the image, the same effect can be achieved for horizontal edges merely by rotating the 3 x 3 kernel of Fig. 7 by ninety degrees before use. If absolute convolutions are used, it does not matter in which direction the rotation is made.

Figure 4 shows several actual edge enhanced processed images according to the present invention. Figure 4a shows an absolute horizontal Sobel convolution. Intensity is simulated by the size of the dot printed at each pixel position. Figure 4b is identical to Figure 4a except that it has been "thresholded", i.e., all pixels having a processed intensity below a threshold value have

-20-

been set to zero (shown as white). In both Figures 4a and 4b, it is easy to see that horizontal edges, for example, at the tips of the toes and the base of the heel have been emphasized, whereas vertical edges, for example  
5 along the edges of the feet, have almost disappeared from view.

In contrast, Figure 4c shows a thresholded absolute vertical Sobel convolution. In this image, the tips of the toes and the heels have almost disappeared while the  
10 vertical edges in the image of the feet are dark and enhanced.

Figure 4d shows a thresholded negative vertical Sobel, similar to an inverted Figure 6b, wherein the absolute value of each image intensity has not been taken  
15 after the convolution, but a thresholding has been completed. The thresholding eliminates all of the negative value points and leaves only one edge visible along the medial or inner edge of the foot. This processing may be used to easily identify only points  
20 along this particular edge of the foot.

Although the 3 x 3 kernel shown in Figure 7 is the preferred kernel, other values in the elements of the kernel may be employed, or the kernel may be expanded to 5 x 5, 7 x 7, etc., which provides further edge  
25 enhancement and smoothing, but substantially slows the speed of the image processing steps.

Continuing now with the description of operation, the captured image has been windowed and split into two subimages, one for each foot. One subimage is then  
30 inverted left for right to form two similar subimages which can be analyzed in the same manner and which have the medial side of the foot always on the right side of the image as seen in Figures 4 and 5.

-21-

In the most highly preferred embodiment, the subimages are then "clipped" before being processed with the Sobel convolution and thresholding operations. "Clipping" is similar to thresholding in that each image pixel is compared to a clipping value which, like the threshold value, is set above the average background level and below the average intensity level of the foot image area. However, in the clipping operation, the intensity of each pixel below the clipping level is increased to the clipping level instead of being reduced to zero as in the thresholding operation.

The clipping operation eliminates the majority of background noise fluctuations without introducing artificial edges or jumps in intensity level between points with intensities just below and points with intensities just above the clipping level.

Although any point of interest may be identified, generally the points identified are points A through G in Figure 5. In order to identify point A, the image is first clipped and then processed as a thresholded absolute horizontal Sobel as shown in Figure 4b. Each row of pixels in the processed subimage is then analyzed as described in the direct analysis procedure starting from the top and working down until the rows containing the enhanced edges are identified.

Although the processing smooths out many noise fluctuations in the raw image, this smoothing also has a tendency to smooth out the sharpness of the edges slightly making it somewhat more difficult to determine the exact edge location. As a result, in the processed image it is very easy to pick out the approximate location of the edge by setting a threshold level and finding all pixels in the searched row of pixels having a value above the threshold. The processing ensures that

-22-

these pixels will be very close to the actual edge location and that a severe location error will not be made. However, due to the inherent smoothing which occurs during the processing, the actual edge location is more difficult to determine accurately. Accordingly, in the preferred embodiment of the invention, after the position of point A is approximately located in the processed image, the original unprocessed captured subimage is examined by the image processor only in the vicinity of the previously identified approximate location for point A to determine the accurate position of point A.

In a similar manner, the location of point B is identified by scanning rows in the processed image starting at the bottom and working upwards.

With the pixel coordinates of points A and B accurately located, the image analyzer provides this information to the computing means which function is also preferably performed by computer 24.

The computing means can then calculate the length of the foot by determining the difference in row numbers between the row of pixels containing point A and the row of pixels containing point B. The scale factor previously determined for the image can then be employed to find the length of the foot in the desired units which may then be converted to shoe size.

In the manner described, each point of interest on the foot can be located and various dimensions of the foot can be calculated. For the purpose of description of this invention, points A through G shown in Figure 5 are located. The relative locations of these points form a "signature" for the foot which may be compared to a database of other stored foot signature patterns to determine the pattern which it most closely resembles.

35



-23-

Because the foot producing each foot signature in the database has been previously carefully analyzed and the results of that analysis have been indexed to each foot signature, the computing means may be used to select the analysis for the matching foot signature. Provided that the signature points are carefully selected, the resulting output will provide an accurate indication of foot shape.

Points A-G have been found to form a suitable signature for selecting shoe size and width, the length of a corrective insert for a shoe and its width at the heel and in the area beneath the ball of the foot. Other points may be added to refine the signature for accurate diagnosis of problems with the foot structure such as pes planus (flat foot), hyperpronation, etc.

To form the signature of points A-G, points A and B are first located in the manner described and the length of the foot is calculated. The width of the heel between points C and D is then determined by examining the thresholded absolute vertical Sobel processed image of Figure 4c.

Points C and D are preferably located by selecting a row of pixels to be analyzed which are a selected percentage of the length of the foot up from the heel point B. In the described embodiment, this selected percentage is 12% of the length of the foot which has been empirically found to give a good indication of heel width for the signature. The row of pixels at the 12% point is then scanned, first in the processed image to identify the approximate location for C and D, then in the unprocessed image to determine final accurate positions.

Point E is located at the head of the first metatarsal. When the foot is properly positioned on the

-24-

support plate, point E will be the point on the perimeter of the foot which is farthest to the right as seen in Figure 5. This point can be identified in the same manner as points A and B by scanning from the right  
5 instead of the top or bottom.

Point F is located approximately 2 mm below point E. This point has also been empirically determined and provides a good point at which the width of the foot can be measured. Next, the image analyzer analyzes the row  
10 of pixels along the line F-G to determine foot width.

As can be seen from the above description, the computer 24 preferably serves all the functions of processing the image to enhance the edges, analyzing the image to locate the points of interest, and computing the  
15 system output.

The computed output is then displayed on the monitor or it may be printed on a printer or other output device. The unprocessed image and the output information are also written onto a disk in the disk drive 26 for  
20 storage in the patient's records.

It will thus be seen that the objects set forth above, among those made apparent from the preceeding description, are efficiently obtained and, since certain changes may be made in the construction set forth above  
25 without departing from the spirit and scope of the invention, it is intended that all matter contained in the above description as shown in the accompanying drawings shall be interpreted as illustrative and not in a limiting sense.

30

35

-25-

What is claimed is:

1. A pedotopography apparatus comprising:  
means for producing a moiré fringe pattern  
representative of the topography of the  
underside of a foot to be analyzed;  
  
image capture means for capturing and storing an  
image of the moiré fringe pattern in an  
image storage buffer;  
  
image analyzing means operatively connected to  
the image capture means for analyzing the  
image of the moiré fringe pattern to  
locate at least two points of interest on  
the foot; and  
  
computing means for calculating information  
corresponding to the distance between the  
two points.
2. A pedotopography apparatus according to claim 1  
further including image processing means for enhancing  
edges in the captured image.
3. A pedotopography apparatus according to claim 2  
wherein the image processing means performs the edge  
enhancement by Sobel convolution.
4. A pedotopography apparatus according to claim 3  
wherein the Sobel convolution is performed with a video  
kernel of 3 x 3 pixels.
5. A pedotopography apparatus according to claim 2  
wherein the image processing means preferentially

-26-

enhances edges which are substantially perpendicular to the centerline of the foot.

6. A pedotopography apparatus according to claim 5 wherein one of the at least two points identified by the image processing means is located at the back of the heel, the other is located at the tip of the forwardmost toe, and the distance between them is calculated by the computing means to determine the length of the foot.

7. A pedotopography apparatus according to claim 2 wherein the image processing means preferentially enhances edges which are substantially parallel to the centerline of the foot.

8. A pedotopography apparatus according to claim 7 wherein one of the at least two points identified by the image analyzing means is located at an inner edge of the foot, the other is located at the outer edge of the foot, and the distance between them is calculated to determine a width of the foot at a selected position.

9. A pedotopography apparatus according to claim 8 wherein the selected position at which the width of the foot is first determined is selected by the computing means which first calculates the length of the foot and then calculates the selected position by taking a predetermined percentage of the calculated length of the foot.

10. A pedotopography apparatus according to claim 9 wherein the width of the foot at the heel is determined by the identifying inner and outer edge points for the foot at approximately twelve percent (12%) of the length of the foot.

-27-

11. A pedotopography apparatus according to claim 8 wherein the selected position at which the width of the foot is determined is selected by the computing means after the image analyzing means identifies a specified point of interest on the foot, said selected position being calculated as a predetermined distance away from the specified point of interest.

12. A pedotopography apparatus according to claim 11 wherein the specified point of interest is located at the base of the first metatarsal.

13. A pedotopography apparatus according to claim 12 wherein the width of the foot is determined approximately two millimeters from the head of the first metatarsal in the direction of the heel of the foot.

14. A pedotopography apparatus according to claim 2 wherein the image analyzing means first analyzes the output of the image processing means containing the enhanced edges to determine approximate positions for the two points and then analyzes the non-edge enhanced image in the vicinity of the approximate positions to determine final accurate positions for the two points.

15. A pedotopography apparatus according to claim 1 wherein the means for producing the moiré fringe pattern representative of the underside of the foot comprises:

a transparent support plate suitable for  
supporting the weight of a person standing  
with at least one foot thereon;

-28-

a grating;

a light source positioned to illuminate the foot from a first direction through the grating whereby a shadow pattern cast by the grating is formed on the underside of the foot; and

a camera positioned to view the foot through the grating from a second direction.

16. A pedotopography apparatus according to claim 15 wherein the camera is positioned such that the second direction from which the camera views the foot is substantially perpendicular to the plane of the support plate.

17. A pedotopography apparatus according to claim 15 wherein the illumination from the light arrives at the foot traveling in the first direction after reflection from an illumination mirror.

18. A pedotopography apparatus according to claim 17 wherein the illumination mirror is adjustable to vary the first direction.

19. A pedotopography apparatus according to claim 15 further including at least one camera mirror in which the camera views the foot from the second direction.

20. A pedotopography apparatus according to claim 19 further including two camera mirrors, one of said camera mirrors being positioned beneath the support plate.

-29-

21. A pedotopography apparatus according to claim 20 wherein the camera mirrors are mounted in a removable tray.

22. A pedotopography apparatus according to claim 15 further including an opaque light shield covering the support plate and the upper surface of the foot and having an opening therein through which the leg of the person projects whereby extraneous light is prevented from entering the camera.

23. A pedotopography apparatus according to claim 22 wherein the opening in the light shield is fitted below the ankle of the person to prevent an image of the ankle or the leg from being seen by the camera.

24. A pedotopography apparatus according to claim 1 further including output means for providing the calculated information to an operator of the pedotopography apparatus.

25. A pedotopography apparatus comprising:

a grating;

a light source positioned to illuminate the underside of a foot from a first direction through the grating;

a camera positioned to view the underside of the foot from a second direction;

image capture means for capturing and storing a first image of the foot from the camera;

-30-

image processing means for processing the first image with an edge-enhancement algorithm to produce a second image;

image analysis means which analyzes the second image of the foot to approximately identify the location of at least two points on the foot and then analyzes the first image in the vicinity of the approximate positions to identify accurate positions for the two points; and

computing means for calculating information corresponding to the distance between the two points.

26. A pedotopography apparatus according to claim 25 wherein the first image contains images of a pair of feet, and the image processing means processes a first windowed portion of the first image, the windowed portion being restricted principally to the portion of the first image containing the image of only one foot.

27. A pedotopography apparatus according to claim 26 wherein the image processing means processes a second windowed portion of the first image, said second windowed portion being restricted principally to the portion of the first image containing the image of the other foot, said second windowed portion being inverted left for right prior to processing.

28. A method for measuring the shape of a foot comprising:



-31-

- (a) producing a moiré fringe pattern representative of the topography of the underside of a foot to be analyzed;
- (b) capturing and storing a first image of the moiré fringe pattern;
- (c) processing the first image to enhance edges thereby forming a second image;
- (d) analyzing the second image to locate at least two points of interest on the foot;  
and
- (e) computing information corresponding to the distance between the two points of interest.

29. A method for measuring the shape of a foot according to claim 28 further including the step of analyzing the first image in the vicinity of at least one of the two points located on the second image to obtain a more accurate location for the at least one point.

Fig. 3

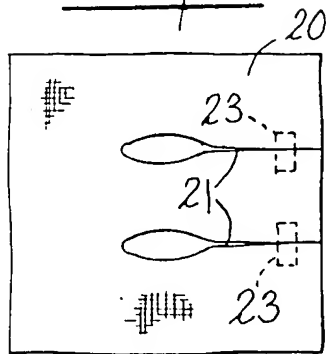


Fig. 1

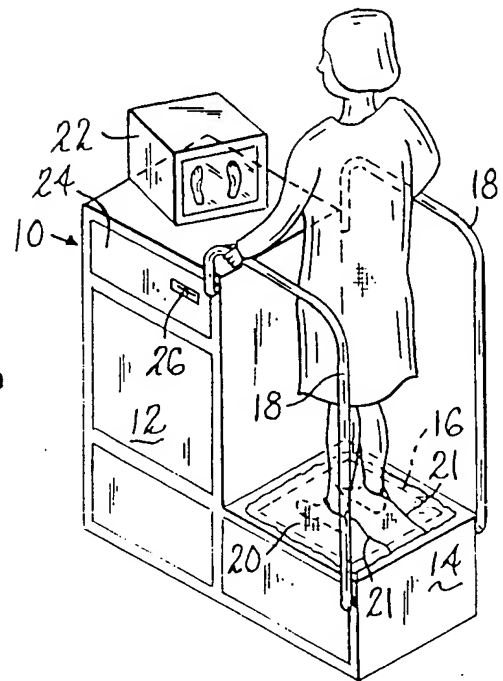
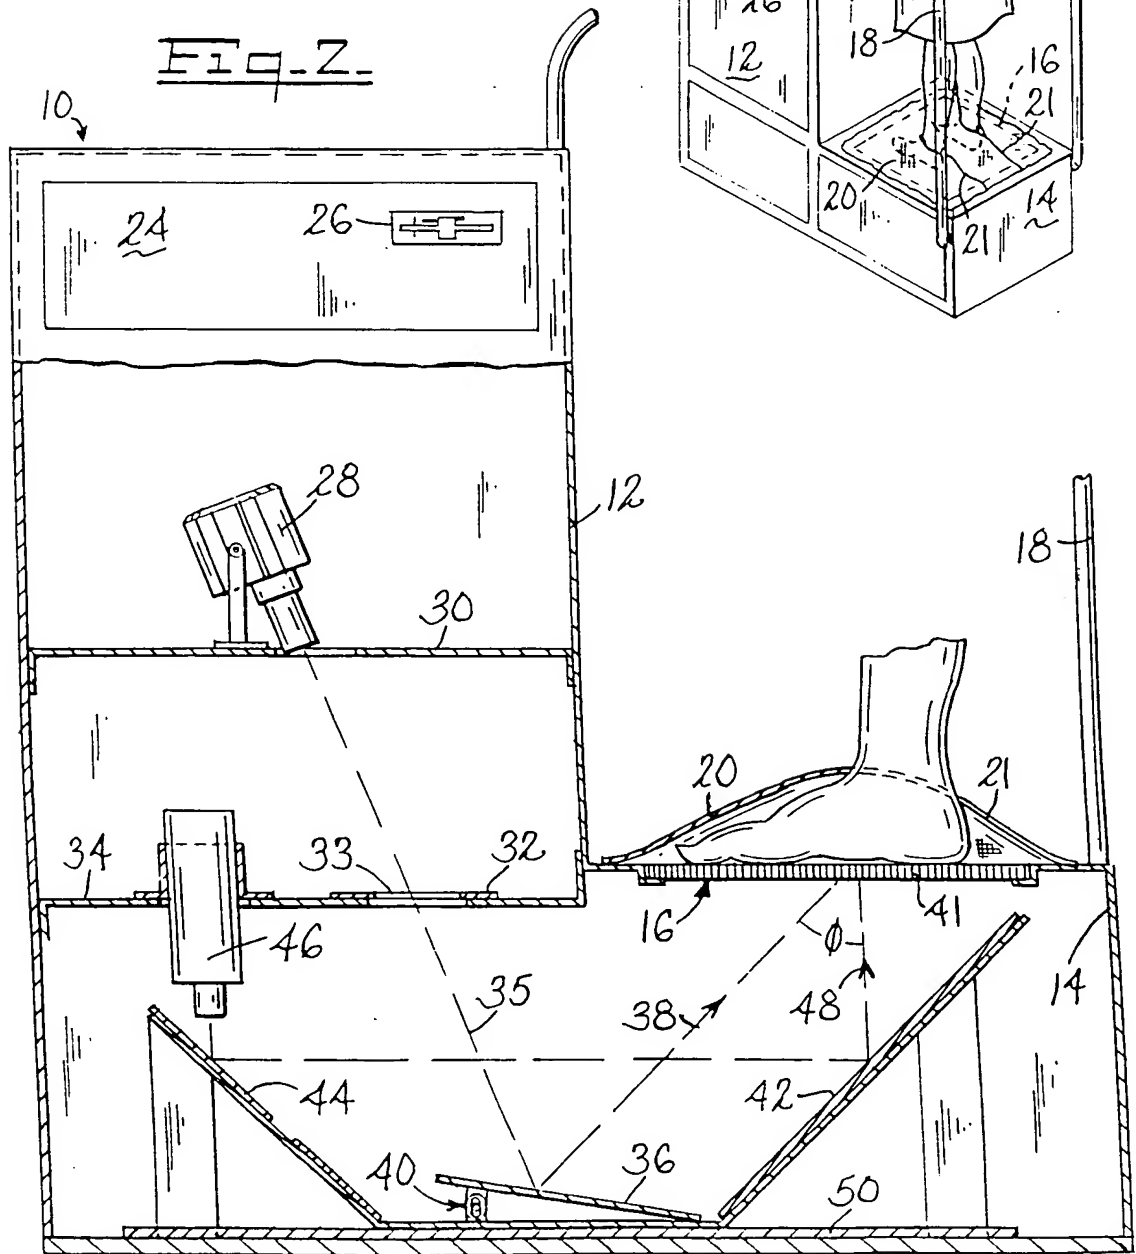


Fig. 2



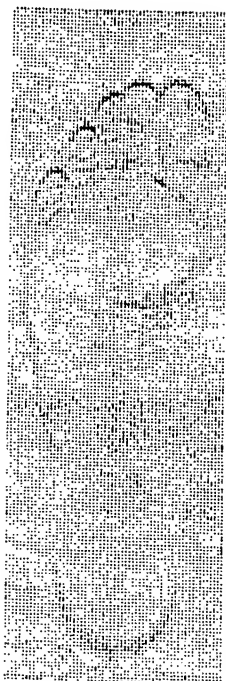


Fig. 4a.

ABSOLUTE HORIZONTAL  
SOBEL



Fig. 4b.

THRESHOLDED ABSOLUTE  
HORIZONTAL SOBEL




Fig. 4c.

THRESHOLDED ABSOLUTE  
VERTICAL SOBEL






Fig. 4d.

THRESHOLDED NEGATIVE  
VERTICAL SOBEL

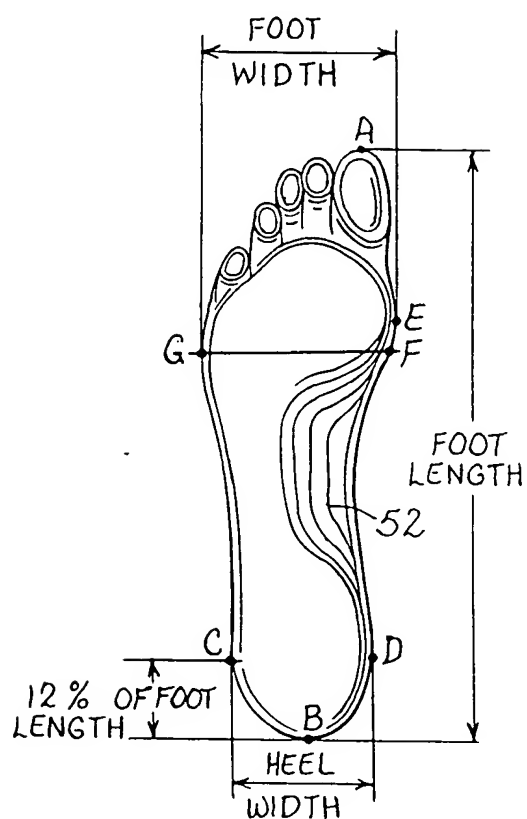Fig. 5.Fig. 7.


3X3  
SOBEL KERNEL

r <sub>1</sub>	-1	0	1
r <sub>2</sub>	-2	0	2
r <sub>3</sub>	-1	0	1
	c <sub>1</sub>	c <sub>2</sub>	c <sub>3</sub>

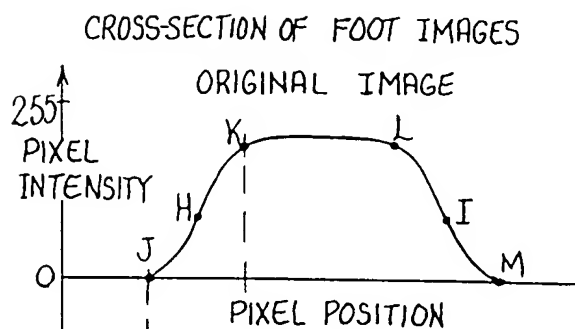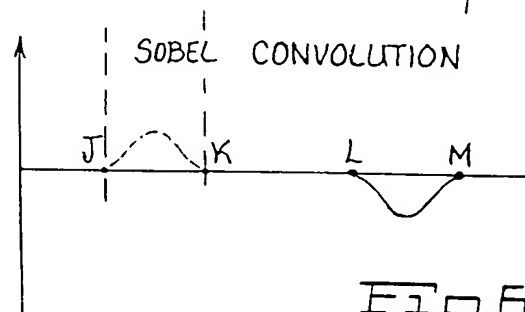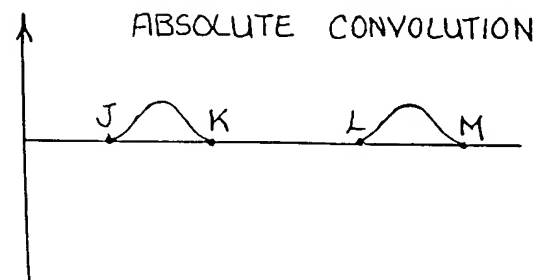Fig. 6a.Fig. 6b.Fig. 6c.

# INTERNATIONAL SEARCH REPORT

International Application No. PCT/US89/04432

<b>I. CLASSIFICATION OF SUBJECT MATTER</b> (if several classification symbols apply, indicate all) <sup>6</sup>		
According to International Patent Classification (IPC) or to both National Classification and IPC IPC(4): G06K 9/00, G01B 11/14 U.S. CL: 382/2, 4; 356/374, 376, 383, 384; 33/3B, C, 515		
<b>II. FIELDS SEARCHED</b>		
Minimum Documentation Searched <sup>7</sup>		
Classification System: <sup>8</sup>	Classification Symbols	
US	382/2, 4 356/374, 376, 383, 384 33/3B, C, 515	
Documentation Searched other than Minimum Documentation to the Extent that such Documents are Included in the Fields Searched <sup>8</sup>		
<b>III. DOCUMENTS CONSIDERED TO BE RELEVANT <sup>9</sup></b>		
Category <sup>10</sup>	Citation of Document, <sup>11</sup> with indication, where appropriate, of the relevant passages <sup>12</sup>	Relevant to Claim No. <sup>13</sup>
A	US, A, 3,627,427 (Johnson) 14 December 1970.	
A	US, A, 2,009,340 (Edwards) 23 July 1935.	
A	US, A, 4,051,483 (Suzuki) 27 September 1977.	
A	US, A, 4,538,353 (Gardner) 03 September 1985.	
A	US, A, 4,541,113 (Seufert et al) 10 September 1985.	
<div style="display: flex; justify-content: space-between;"> <div style="width: 45%;"> <p><sup>*</sup> Special categories of cited documents: <sup>10</sup></p> <p>"A" document defining the general state of the art which is not considered to be of particular relevance</p> <p>"E" earlier document but published on or after the international filing date</p> <p>"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</p> <p>"O" document referring to an oral disclosure, use, exhibition or other means</p> <p>"P" document published prior to the international filing date but later than the priority date claimed</p> </div> <div style="width: 45%;"> <p>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</p> <p>"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step</p> <p>"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.</p> <p>"&amp;" document member of the same patent family</p> </div> </div>		
<b>IV. CERTIFICATION</b>		
Date of the Actual Completion of the International Search		Date of Mailing of this International Search Report
04 December 1989		22 JAN 1990
International Searching Authority		Signature of Authorized Officer
ISA/US		 Michael Razavi

HI DOCUMENTS CONSIDERED TO BE RELEVANT (CONTINUED FROM THE SECOND SHEET)		
Category	Citation of Document, with indication, where appropriate, of the relevant passages	Relevant to Claim No.
A	US, A, 4,604,807 (Bock et al) 12 August 1986.	
A	US, A, 4,525,858 (Cline et al) 25 June 1985.	